pH SOLUTIONS

CERTIFICATE OF ANALYSIS

260831-899-NHS-1

Issued Oct 27, 2026

SAMPLE

KLOW 80mg

Prepared for **NuLumin** · Lot **NUL-KLW80-20260824-01**

PASS

ISO/IEC 17025:2017 ACCREDITED

A2LA R243 · PJLA Testing #84351 · Zero recalls since 2016

181 W Huntington Dr, Suite 181, Monrovia, CA 91016 · (818) 808-9757

BATCH / LOT	SAMPLE ID	MATRIX	PANELS RUN
NUL-KLW80-20260824-01	260831-899-NHS-1	Peptide	3

RECEIVED	REPORTED	CLIENT
Aug 31, 2026	Oct 27, 2026	NuLumin

PEPTIDE PURITY

ANALYTE	RESULT	UNIT	LIMIT / METHOD	STATUS
KLOW — purity	99	%	HPLC-UV @ 220 nm	PASS

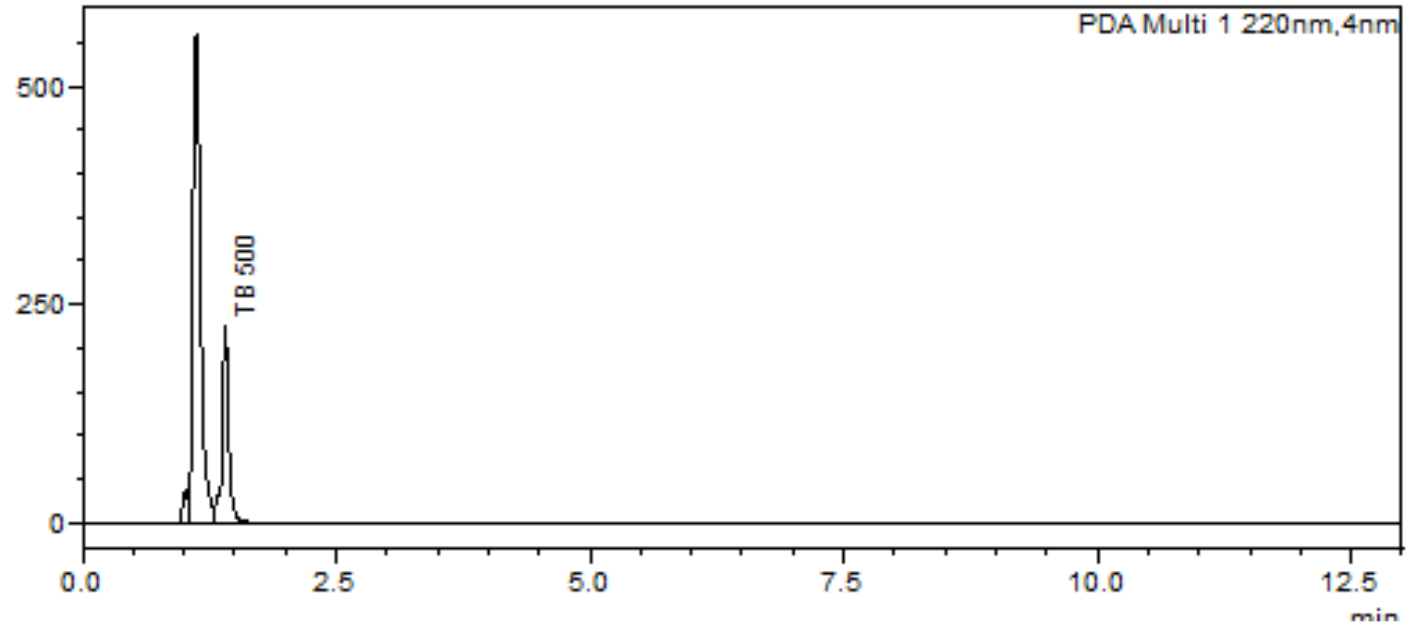
WATER ACTIVITY

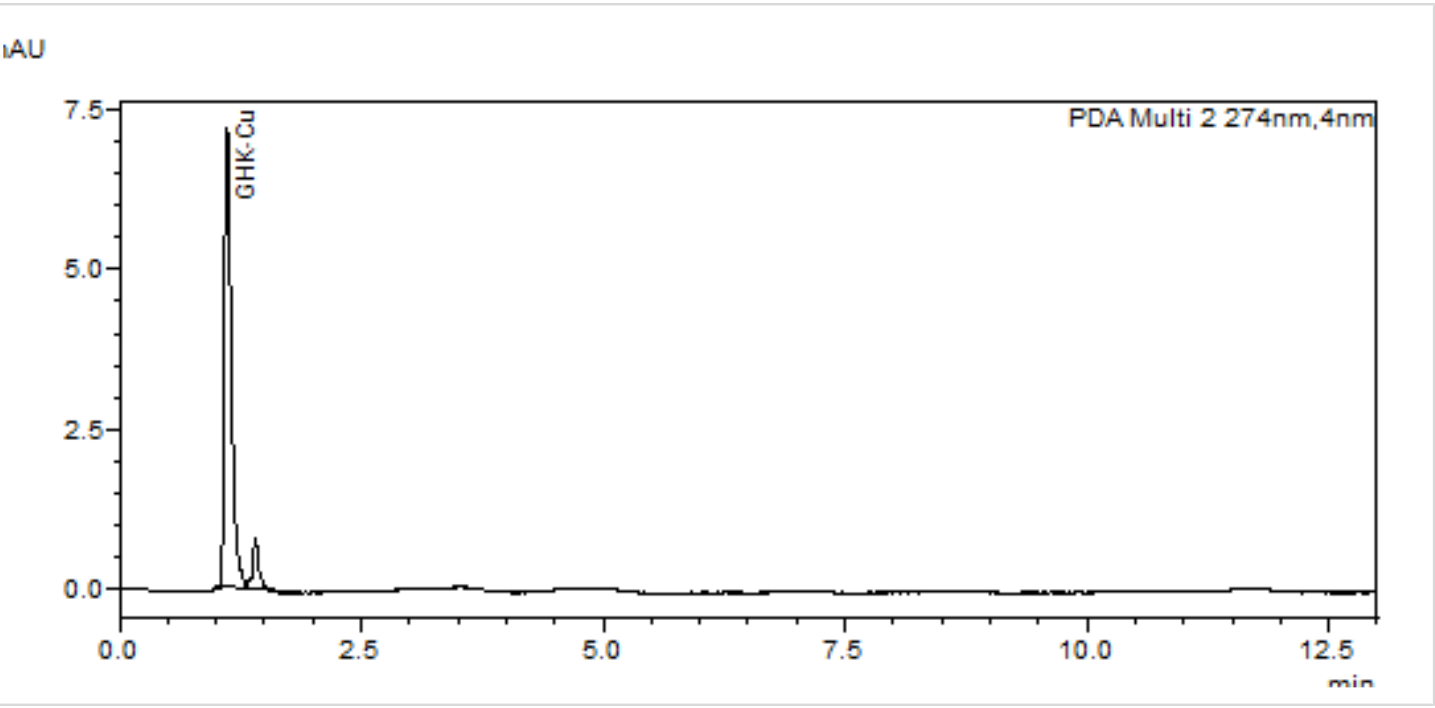
ANALYTE	RESULT	UNIT	LIMIT / METHOD	STATUS
Water activity	0.19	aw	< 0.65	PASS

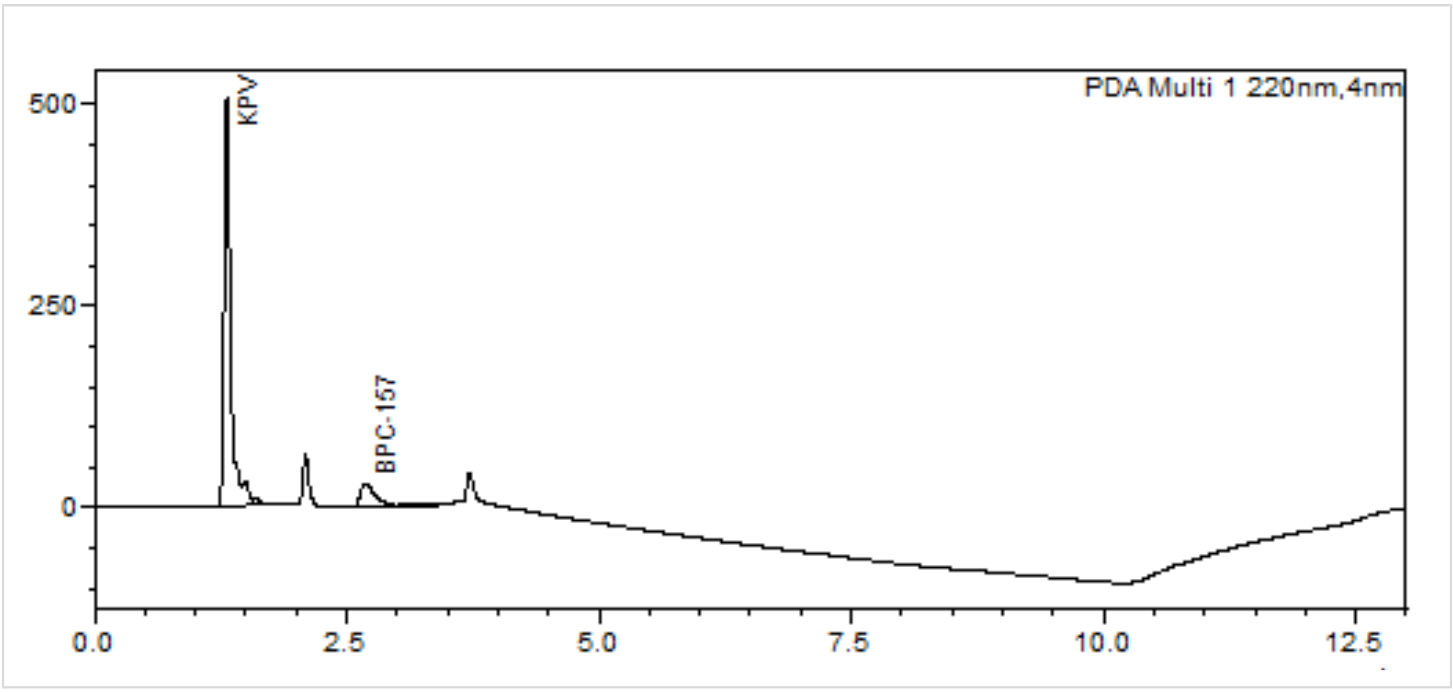
MICROBIALS

ANALYTE	RESULT	UNIT	LIMIT / METHOD	STATUS
E. Coli	Not Detected		Not detected in 1 g	PASS
Salmonella spp.	Not Detected		Not detected in 1 g	PASS
Aspergillus flavus	Not Detected		Not detected in 1 g	PASS
Aspergillus fumigatus	Not Detected		Not detected in 1 g	PASS
Aspergillus niger	Not Detected		Not detected in 1 g	PASS
Aspergillus terreus	Not Detected		Not detected in 1 g	PASS

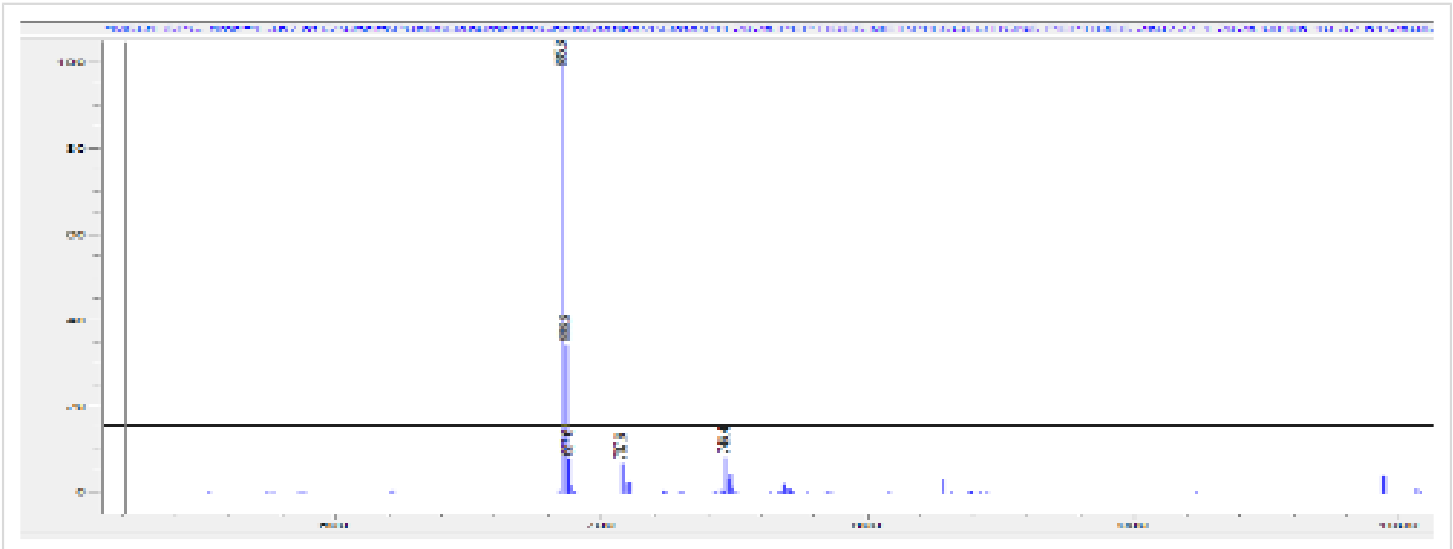
CHROMATOGRAMS


PDA Multi 1 220nm,4nm
500
250
0
TB 500
0.0
2.5
5.0
7.5
10.0
12.5
min


mAU
PDA Multi 2 274nm,4nm
7.5
5.0
2.5
0.0
GHK-Cu
0.0
2.5
5.0
7.5
10.0
12.5
min


PDA Multi 1 220nm,4nm
500
250
0
KPV
BPC-157
0.0
2.5
5.0
7.5
10.0
12.5





PH SOLUTIONS LAB INC.

Analysis performed in accordance with ISO/IEC 17025:2017. Results relate only to the sample as submitted. This certificate may not be reproduced except in full without the written approval of the laboratory. The online copy at the address beside is authoritative: if a printed COA disagrees with it, the online copy governs. Questions: info@phsolutionslab.com · (818) 808-9757.

SCAN TO VERIFY

www.phsolutionslab.com/c/eyJjIjoiMjYwODMxLTg5OS1OSFMtMSIsInAiOiJOdUx1bWluIiwibCI6Ik5VTC1LTFc4MC0yMDI2MDgyNC0wMSJ9.1DG5Hz-YGPX3UpIxaUrcL483SYdW0z25